



Micro TM



SoftwareUser Guide



Table of Contents

TranscendSoftwareUserGuide	3
Configuration	5
Compliance Manager	7
General Functions	8
Contact Transcend Inc.	12


Transcend Software User Guide

Your Transcend Micro device comes with easy-to-use software to help adjust settings, observe, print and send reports, and store all your data so you can access it any time.

Three Simple Steps and you're ready to use your software.


STEP 1

- Start by downloading the device software onto your computer. Once you download the software, it will automatically update as changes and improvements are made to the software.
 - o Software download link: mytranscend.com/software
- When you open the software, the home screen will appear.

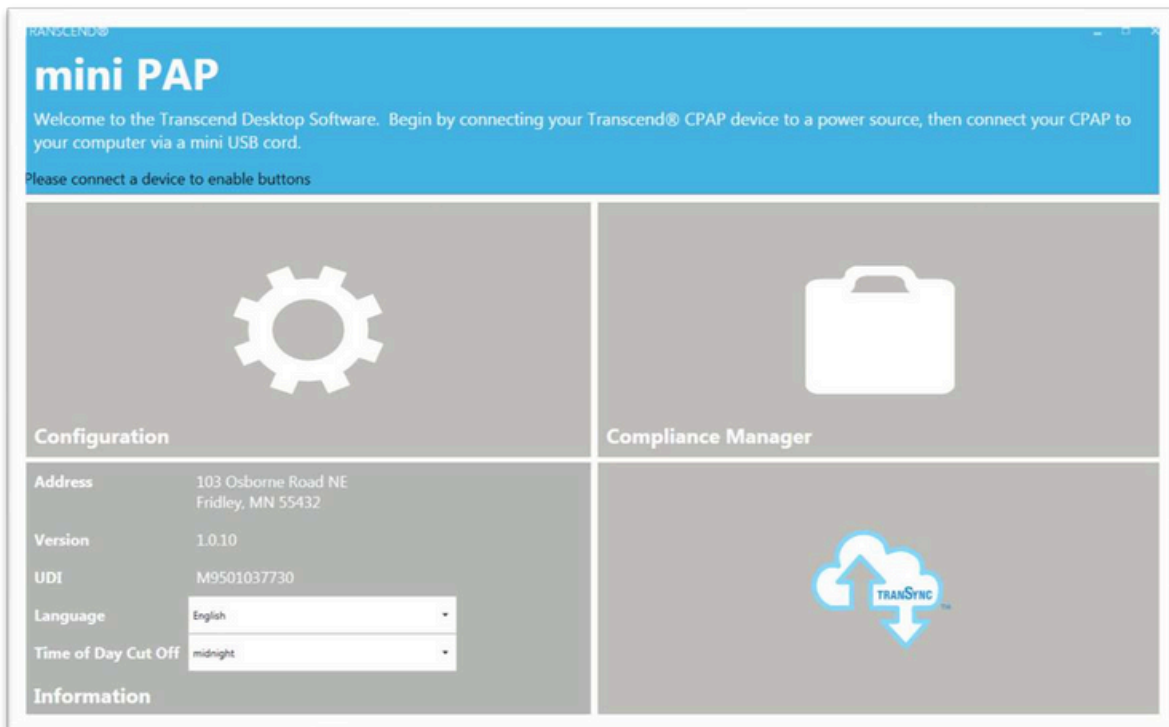


STEP 2

Connect your Transcend Micro device to a power source, then connect it to your computer using a USBC data cord. Connect only to certified IEC 60950 or IEC 60601 computers.

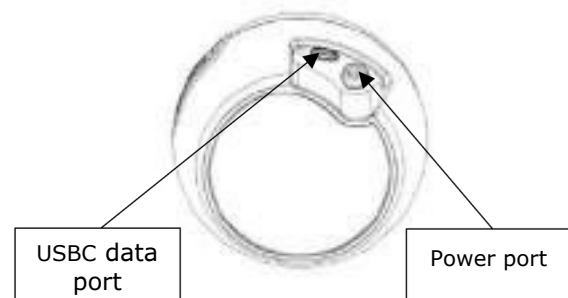

STEP 3

- Select your preferred language by choosing from the dropdown menu.
- Select your Time of Day Cut Off from the dropdown menu. This will be used to group sleep sessions into 24-hour days. Choose a time when you are least likely to be sleeping.

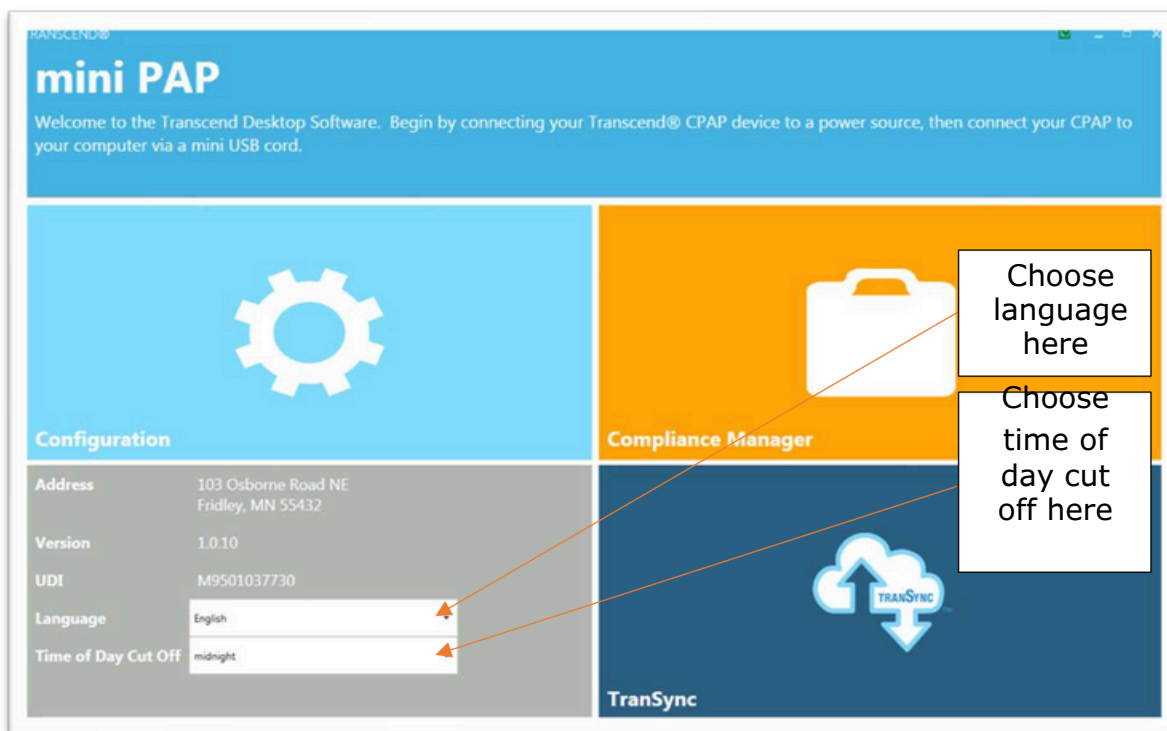

Now You're Ready to Use the Transcend Desktop Software

On the Home screen interface, there are two primary areas to choose from: Configuration or Compliance Manager. Let's explore each one.

NOTE: If you disconnect your CPAP from a power source while in the software program, the software will return to the home screen until power is resupplied. Any unsaved settings will be lost.

Configuration

Select the Configuration box to open the configuration settings application.

Notice that when you are on any screen, in the right upper corner you will see icons for the available applications in the software. Simply click on any of them and you will go directly to that section.



The Configuration area is used to adjust various settings on the device.

Some features, such as the Therapy Pressure and Calibration are clinician settings and are only available with a password.

You can, however, adjust the Ramp Starting Pressure, Ramp Duration and EZEX pressure relief settings if these options have been set by your clinician to be adjustable.

To change them, simply slide on the red oval across the line to the right or left.

- **Therapy Pressure is a clinician setting** that can only be accessed with a password.
- **Ramp Starting Pressure** controls the pressure at which your CPAP therapy starts when you engage the Ramp feature. This selection can be adjusted up to 1cmH20 below your Therapy Pressure.

- **Ramp Duration** control show long it takes for your CPAP to reach your prescribed therapy pressure when the Ramp feature is engaged. The Ramp feature provides you with a lower therapy pressure to help you fall asleep more comfortably as it slowly ramps the CPAP pressure up to your prescribed therapy level. This setting can be adjusted between 5 and 45 minutes or toggle the switch to OFF to deactivate this feature.
- **EZEX Setting** drops the pressure as you breathe out to make exhalation while using your CPAP more comfortable for you. This can be set to OFF, or pressure relief settings between 1 and 3 (3 being the greatest amount of pressure relief).
- **Calibrate feature is a clinician setting** that can only be accessed with a password. To calibrate the device, first make the appropriate adjustments to the other CPAP settings and click the update button. You will not be able to calibrate the device while you are adjusting the other CPAP settings until you click update. Connect the mask tubing and a manometer to the CPAP and power on the machine. If calibration is needed, select the calibrate button and slide the setting to the appropriate level. Click the calibrate complete button when finished.
- **NOTE: To SAVE your adjustments to your CPAP settings, click the [update](#) button (next to the calibrate button on your screen) before navigating to another screen.**

Compliance Manager

Because both you and your clinician have an interest in the quality of your sessions, the **Compliance Manager** generates summary data and reports so you can review your sessions by day, week, month or longer.



You can see the primary data summaries are:

- Usage
- Leak Summary
- Pressure Summary
- AHI-Events per Hours of Use
- Patient Therapy Settings

General Functions

Filtering by Date

Tailor the date range of information by clicking on the calendar icons next to choose the desired start and end dates.

Then click the Filter button to update the start and end dates you would like to view.

The screenshot shows a web interface for date filtering. At the top, there are two date pickers: 'Start Date' set to 9/25/2018 and 'End Date' which has a calendar dropdown open. The calendar is for September 2018, with the 25th highlighted. Below the date pickers is a 'Filter' button. Underneath, there is a summary table for usage:

Usage Category	Count	Percentage
4-6 Hours Usage	9	18%
6-8 Hours Usage	16	33%
8+ Hours Usage	23	47%
Not Used	43 of 49 days	(88%)

Below this table is a section titled 'PRESSURE SUMMARY' with a single entry: 'Average Pressure' is 5.6 (cmH2O).

Generate Compliance (Last 30 days of compliance report)

The 30-Day Compliance button will automatically pull the last 30-day window of compliance data that has at least 70% compliance (4+ hours of therapy 70% of the time).

The screenshot shows the '30 Day Compliance' report interface. At the top right, there are icons for settings (gear) and a folder. The main section has two date pickers: 'Start Date' set to 9/25/2018 and 'End Date' set to 11/13/2018, with a 'Filter' button between them. To the right of the date pickers are two buttons: '30 Day Compliance' and 'Export Report'. Below this is a table showing usage data for the 30-day period:

Usage Category	Count	Percentage
4-6 Hours Usage	0 of 49 days	(0%)
6-8 Hours Usage	0 of 49 days	(0%)
8+ Hours Usage	0 of 49 days	(0%)

Export Report

When you choose Export Report, you can save the data you are currently viewing on your screen as a .pdf document on your computer.

You will see the following screen after choosing Export Report. Type in the info you wish to save with your report: your name, address, provider name, provider phone and select a location for the .pdf to be stored on your computer. Desktop is recommended as an export location since the file will be easy to locate. Click [export report](#) button to save your report as a pdf. Once it's saved, you can click on the .pdf document to view or print it from your computer.

The screenshot shows the 'Compliance Manager' interface with a modal form for exporting a report. The form is titled 'SELECT / PROVIDER INFORMATION' and contains the following fields:

- Serial Number: 818020111
- Patient Name:
- Address:
- Provider Name:
- Provider Phone:
- Export Location: (with a dropdown menu showing 'Desktop' selected)


Below the form, there are two buttons: 'cancel' and 'export report'. At the bottom of the screen, there is a table with compliance data:

Compliance Index	Max	Min	Max
Time to Apnea	0%	20 min/20	20 min/20
Time to Hypoxemia	0%	20 min/20	20 min/20
Time to Hypoxemia	0%	20 min/20	20 min/20

At the top of the page you will also see three grey tabs: Daily List, Trend Graph and Day Graph.

The screenshot shows the 'Compliance Manager' interface with the 'Daily List' tab selected. The page has a blue header with the 'TRANSCEND' logo and a back arrow. Below the header, there are four tabs: 'Compliance Summary', 'Daily List', 'Trend Graph', and 'Day Graph'. The 'Daily List' tab is active, showing a 'FILTER' section with a 'Device Serial' field containing the value '818020111'.

Daily List

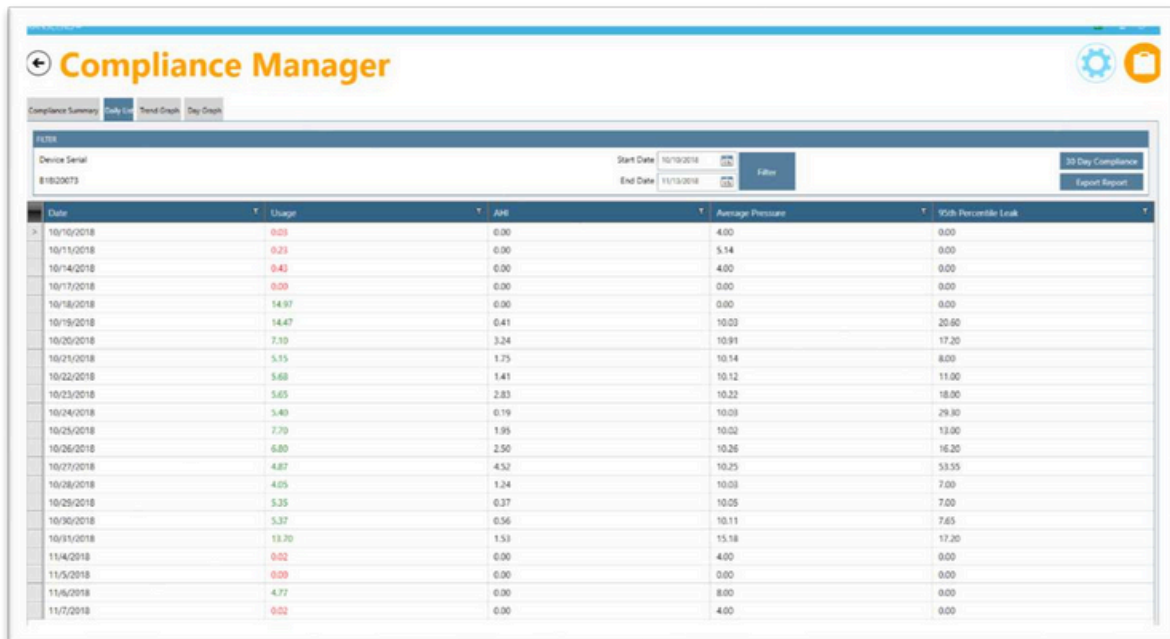


The screenshot shows the 'Compliance Manager' interface with the 'Daily List' tab selected. The table displays data for device serial 81802073 from 10/10/2018 to 11/7/2018. The columns are Date, Usage, AHI, Average Pressure, and 95th Percentile Leak.

Date	Usage	AHI	Average Pressure	95th Percentile Leak
10/10/2018	0.03	0.00	4.00	0.00
10/11/2018	0.23	0.00	5.14	0.00
10/14/2018	0.43	0.00	4.00	0.00
10/17/2018	0.00	0.00	0.00	0.00
10/18/2018	14.97	0.00	0.00	0.00
10/19/2018	14.47	0.41	10.03	20.60
10/20/2018	7.10	3.24	10.91	17.20
10/21/2018	5.15	1.75	10.14	8.00
10/22/2018	5.68	1.41	10.12	11.00
10/23/2018	5.65	2.83	10.22	18.00
10/24/2018	5.40	0.19	10.08	29.30
10/25/2018	7.70	1.95	10.02	13.00
10/26/2018	6.80	2.50	10.26	16.20
10/27/2018	4.87	4.52	10.25	53.55
10/28/2018	4.05	1.24	10.03	7.00
10/29/2018	5.35	0.37	10.05	7.00
10/30/2018	5.37	0.56	10.11	7.65
10/31/2018	13.70	1.53	15.18	17.20
11/4/2018	0.02	0.00	4.00	0.00
11/5/2018	0.00	0.00	0.00	0.00
11/6/2018	4.77	0.00	8.00	0.00
11/7/2018	0.02	0.00	4.00	0.00

When you select the Daily List tab you will see a general summary for the date range you have indicated. Daily List shows the Date, Hours Used, Average AHI (Apnea Hypopnea Index), Average Pressure and Average Leak percentile for each therapy session. You can reverse the order of the data shown by selecting the column header you (Date, Usage, AHI, Average Pressure or 95th Percentile Leak).

Trend Graph

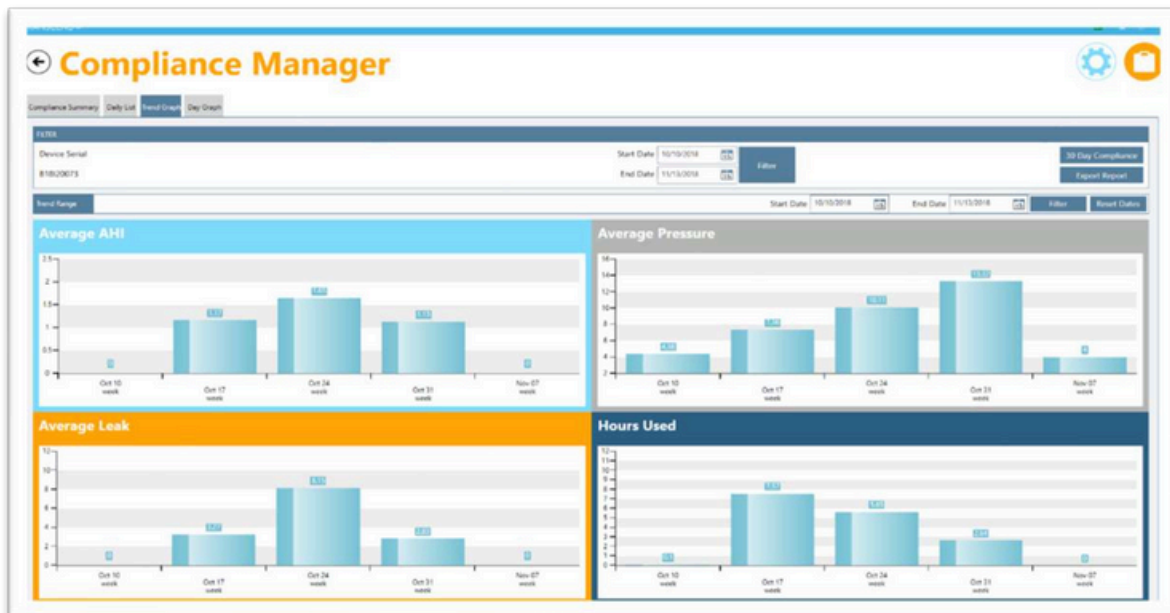


When you click the Trend Graph tab at the top of the page, you'll see the data in graphic form. Click on any bar graph and you will see trend ranges by month, week or day each time you click (this change in date range is reflected in the Trend Range section).

At any time, you can adjust the date range you want to view by changing the date range and clicking the Filter button. You can reset the date range after you've finished drilling down by hitting the [Reset Dates](#) button.

Day Graph

Select the Day Graph tab is used to show data that has been drilled down to the day in the Trend Graph tab or you can go to this tab to select a particular day's data. You can choose the day you would like to view by selecting the date in the Selected Date field.

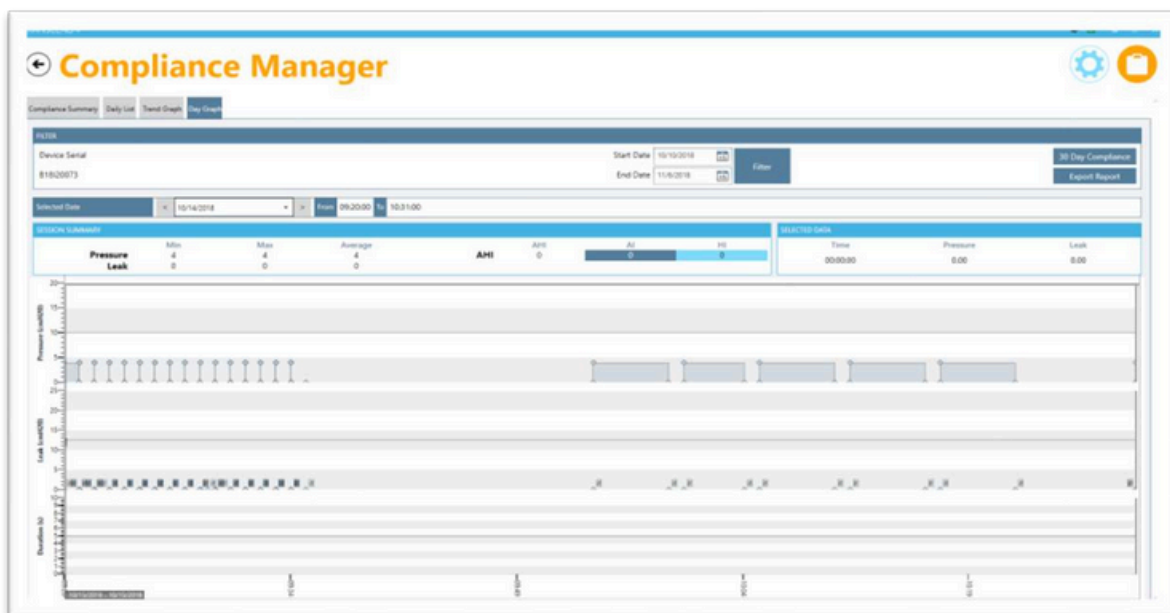

Contact Transcend Inc.

Corporate headquarters	Transcend	Inc.
Email	customersupport@mytranscend.com	
Web	http://www.MyTranscend.com/	
Telephone	651.621.1800	877.621.9626
Toll-free telephone	651.204.0064	
Fax	Transcend Inc. 103 Osborne Road NE Fridley, Minnesota 55432 USA	



104207 Rev A 2022-05

NOTE: For more detailed descriptions, warnings, cautions and troubleshooting procedures refer to the Transcend Micro User Manual that is available for download at www.MyTranscend.com/support or by calling Transcend customer service at 877-621-9626 to request a copy.